

Report on Testing of AMwand and Pendant (Amized Fusion Technology devices) by Amega Global

Live-Blood Analysis

February 25th, 2010

General Description:

The AMwand (manufactured by Amega Global) is a device containing *AMized Fusion Technology (AFT)*, a proprietary name referring to the wands emitting a beam of *zero point field energy* resonance.

The live-blood analysis was done using a NIKON Microscope Eclipse 50i, which enlarges the sample 17,000 times. The microscope was connected to a large computer screen, so all those present were able to observe the images.

Subjects and Witnesses Present during the Testing:

An experienced practitioner operating the equipment, a volunteer whose blood sample was analyzed before and after the application of AFT, three people applying the energy, and a cameraman filming the session were present in the room.

Procedure:

Blood was taken from the volunteer's finger as a baseline, and various imprints were put under the microscope. Several images of the state of his blood were observed. One of the images is seen below in Figure 1.

Figure 1 shows the red blood cells clumped together (a sign of lack of oxygen). In vivo, it was also clear that the white blood cells were not moving (i.e., low immune system activity).

Next, the volunteer received the application of AFT with 3 wands for 3 minutes. The areas of application were above his head, on the palm of his left hand, and over his abdomen. The subject also wore an Amega Global pendant with AFT around his neck.

Following, blood was taken again from the same volunteer's finger and the imprints were put under the microscope. Several images of the state of his blood were observed, including the image shown below in Figure 2.

Figure 2 shows that after three minutes of application of AFT, the red blood cells are clearly differentiated, as in any normal blood sample. There is also more light in the center of the cells, indicated increased oxygen. In vivo, all witnesses could see that the white blood cells were now moving (i.e., the immune system had been activated).

Baseline:

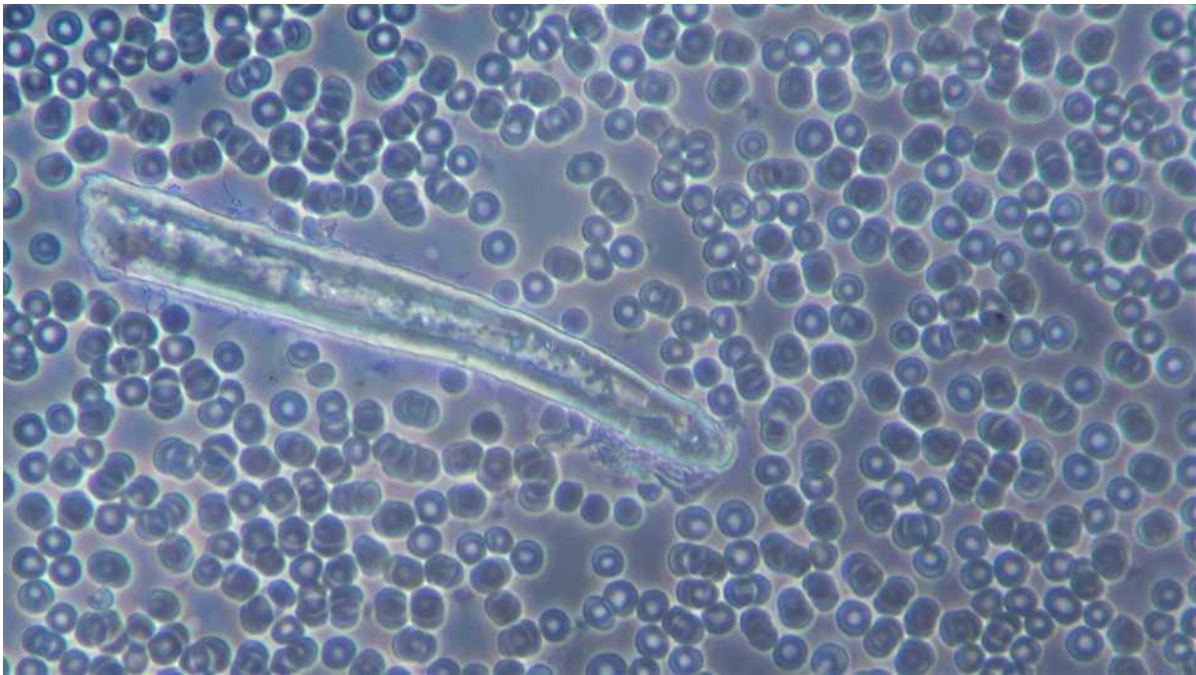


Figure 1. This image shows the red blood cells clumped together (a sign of lack of oxygen). In vivo, it was also clear that the white blood cells were not moving (i.e., low immune system activity).

Results:

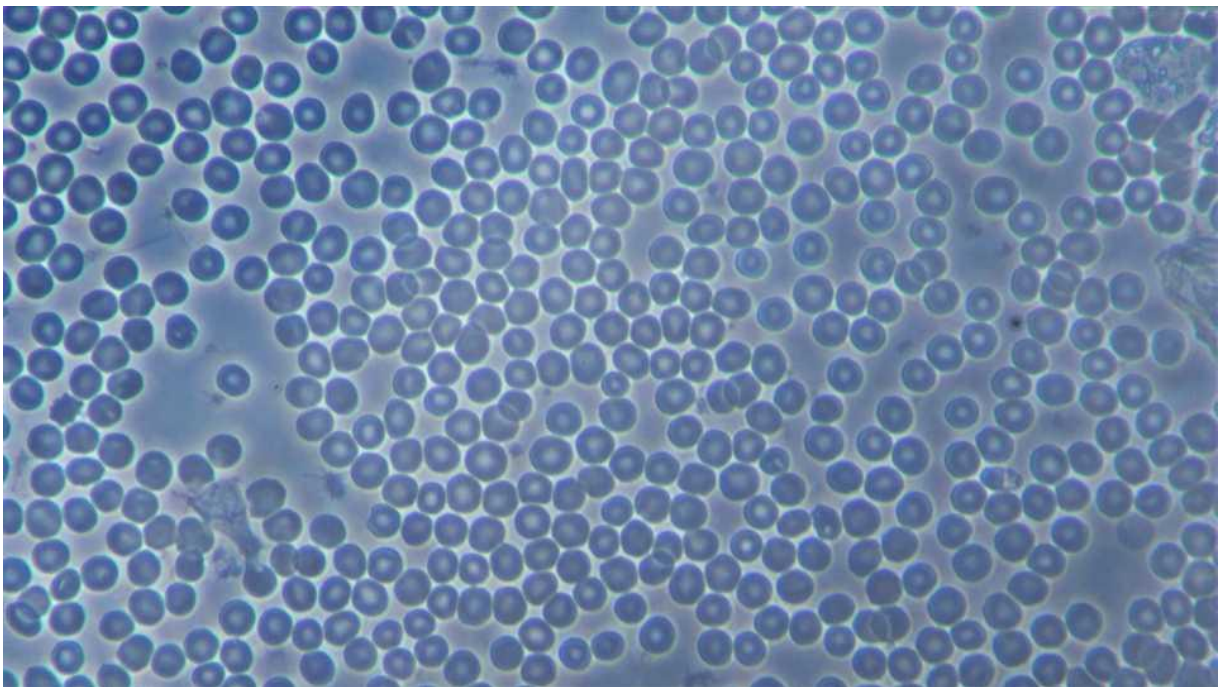


Figure 2. This image shows that after three minutes of application of AFT, the red blood cells are clearly differentiated, as in any normal blood sample. There is also more light in the center of the

cells, indicated increased oxygen. In vivo, all witnesses could see that the white blood cells were now moving (i.e, the immune system had been activated).

Discussion:

As the before and after images show, the live-blood samples of our volunteer rapidly increased in healthy appearance after only 3 minutes of application of AMized Fusion Technology.

These results appear to support Amega Global's explanation that the AMwand and other AMized Fusion Technology products can rapidly energize the human electromagnetic field and body (as well as all other organic matter) to promote health. It is hypothesized that the supply of the frequencies contained in AFT to the organism in this manner induces a state of homeostasis, or balance. This is what triggers the natural self-healing mechanism of each individual to produce the changes necessary for cellular and/or energetic repair and improvement.

There appears to be a strong correlation between this process and the experiential results observed by many during the live demonstrations being organized by the company's independent distributors to show the effects that this technology has on immediate pain relief, increase in strength and flexibility, and the positive changes detected in the taste of food, water, wine, etc.